


INSTRUCTION MANUAL

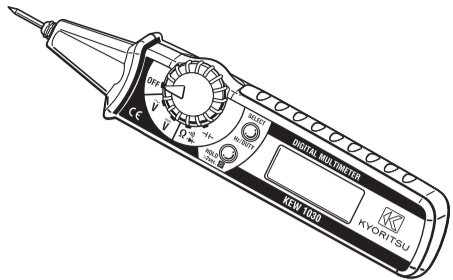

PEN TYPE DIGITAL MULTIMETER KEW 1030

KYORITSU ELECTRICAL INSTRUMENTS
WORKS, LTD.

3-25 92-1634K

1. Safety warnings

This instrument has been designed, manufactured and tested according to IEC 61010: Safety requirements for Electronic Measuring apparatus, and delivered in the best condition after passed the inspection.

This instruction manual contains warnings and safety rules which must be observed by the user to ensure safe operation of the instrument and retain it in safe condition. Therefore, read through these operating instructions before using the instrument.

WARNING

- Read through and understand the instructions contained in this manual before using the instrument.
- Save and keep the manual at hand to enable quick reference whenever necessary.
- The instrument is to be used only in its intended applications.
- Understand and follow all the safety instructions contained in the manual.
- The RESPONSIBLE BODY shall be made aware that, if the equipment is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.
- Failure to follow the instructions may cause injury, instrument damage and/or damage to equipment under test. Kyoritsu is by no means liable for any damage resulting from the instrument in contradiction to this cautionary note.

The symbol Δ indicated on the instrument means that the user must refer to the related parts in the manual for safe operation of the instrument. Be sure to carefully read the instructions following each Δ symbol in the manual.


- DANGER** : is reserved for conditions and actions that are likely to cause serious or fatal injury.
- WARNING** : is reserved for conditions and actions that can cause serious or fatal injury.
- CAUTION** : is reserved for conditions and actions that can cause injury or instrument damage.

Please refer to following explanation of the symbols used on the instrument and in this manual.

Δ	User must refer to the explanations in the instruction manual.
	Instrument with double or reinforced insulation
~ AC	AC
DC	DC
	This instrument satisfies the marking requirement defined in the WEEE Directive (2002/96/EC). This symbol indicates separate collection for electrical and electronic equipment.

4-3 Method of storing the test lead

Test lead is stored in the rear side compartment of the instrument. Cord is wound around the cord holder.



5. Functions

Auto-ranging (AUTO)
A function to automatically select the appropriate measurement range based on the input signal. The "AUTO" mark is displayed on the LCD while this function is activated. This function is not available in Diode check, Continuity check and Duty ratio measurements. The "AUTO" mark is not displayed.

Hold function (H)
A function to freeze the measured value on the LCD. (Not available in Frequency measurement)
The "H" mark is displayed on the LCD when the HOLD key is pressed. Then the measured value is frozen. Press this key again or switch the measurement function to others to release the Hold function.

REL function (Δ)
A function to display the difference between the measured values (relative value) on the LCD at DCV and Capacitance functions. The " Δ " mark is displayed on the LCD when the HOLD key is pressed. Then the value being measured is stored. After that, the difference between the stored value and the measured value is displayed on the LCD. Press this key again or switch the measurement function to others to release the REL function.

Auto-power-off function
A function to turn off the instrument when 30 min. have elapsed after the Function switch is switched from OFF to the other measurement function. Press the HOLD key again or switch the measurement function to others to restore from the Auto-power-off state.

Over-range indication
When the measured value exceeds the max. indication range, "OL" is displayed on the LCD. (This indication is not displayed at AC/DC 600V range.) This indication is not displayed while the Hold function is activated.

Low battery warning (BATT)
When the battery voltage drops to 2.4V±0.2V or less, the "BATT" mark is displayed on the LCD.

Penlight
Set the Function switch to "LIGHT" position to turn on the Penlight. Turn the switch to any desirable function position. (Measurement cannot be performed when the switch is in "LIGHT" position.) Turn the switch to "OFF" position to turn off the light.

LCD backlight
The LCD backlight lights up by pressing down the HOLD key at any measurement function other than OFF at least 2 sec. Press down this key again at least 2 sec. or turn the Function switch to OFF once to turn off the light.

Note
Penlight and LCD backlight are not turned off automatically. Be sure to turn them off when they are not in use.
When turning on/off the LCD backlight, the "H" mark is displayed on the LCD and the Hold function is activated. Press the HOLD button for a while to release the function and perform the next measurement.

6. Measurement

DANGER

- To prevent electrical shock to person and damage to the instrument, following instructions must be observed.
- The max. rated voltage to ground is AC/DC600V. Never attempt to make measurement on a circuit in which electrical potential to the ground exceeding this voltage exists.
- The max. input voltage is DC600V/AC600Vrms (sin). Never attempt to make any measurement on a circuit in which electrical potential exceeding this voltage exists.
- Do not operate the Function switch during a measurement.
- Never make a measurement with the Bottom case is removed.
- Keep your fingers and hand behind the barrier (see 4-1) of the instrument and test lead.
- Be careful not to short-circuit the line under test with the metal part of the instrument or the test lead during a measurement.
- Never make measurement on an energized circuit at Resistance, Diode check, Continuity check and Capacitance function of this instrument.
- Always attach the cap firmly when using the test lead under CAT III environment. When the test lead is connected to the instrument, the lower category either of them belongs to is applied.
- Keep your fingers and hands behind the protective fingerguard during measurement.

Read through the following safety instructions contained in this manual before using the instrument.

DANGER

- Never make measurement on a circuit in which electrical potential to ground over 600V exists.
- Do not attempt to make measurement in the presence of flammable gases. Otherwise, the use of the instrument may cause sparking, which can lead to an explosion.
- Never attempt to use the instrument if its surface or your hand is wet. Otherwise, you may get electrical shock.
- Never open the Bottom case and Battery cover during a measurement.
- Do not exceed the maximum allowable input of any measuring range.
- Never try to make measurement if any abnormal conditions, such as broken case is noted.
- The instrument should be used only in its intended applications or conditions. Otherwise, safety functions equipped with the instrument do not work, and instrument damage or serious personal injury may be caused.
- Verify proper operation on a known source before use or taking action as a result indication of the instrument.
- Keep your fingers and hands behind the protective fingerguard during measurement.

WARNING

- Never attempt to make any measurement if any abnormal conditions, such as broken case and exposed metal parts are present on the instrument or test lead.
- Do not install substitute parts or make any modification to the instrument. Return the instrument to your local Kyoritsu distributor for repair or re-calibration.
- Do not turn the function switch with plugged in test leads connected to the circuit under test.
- Do not try to replace the batteries if the surface of the instrument is wet.
- Always switch off the instrument before opening the battery compartment cover for battery replacement.
- Stop using the test lead if the outer jacket is damaged and the inner metal or color jacket is exposed.

CAUTION

- Always set the Function switch to the appropriate position before making measurement.
- Do not expose the instrument to the direct sun, high temperatures and humidity or dew.
- This instrument is designed for in-door use. It can be used under the temperature between 0°C and 40°C without impairing its safety characteristics.
- This instrument doesn't have dust/water-proof construction. Do not use the instrument in dusty area or where it easily gets wet. It may lead to failure of the instrument.
- Be sure to set the function selector switch to the "OFF" position after use. When the instrument will not be in use for a long period of time, place it in storage after removing the battery.
- Use a damp cloth and detergent for cleaning the instrument. Do not use abrasives or solvents.

Measurement categories (Over-voltage categories)
To ensure safe operation of measuring instruments, IEC61010 establishes safety standards for various electrical environments, categorized as O to CAT IV, and called measurement categories. These are defined as indicated below. Higher-numbered categories correspond to electrical environments with greater momentary energy, so a measuring instrument designed for CAT III environments can endure greater momentary energy than one designed for CAT II.

- CAT II : Primary electrical circuits of equipment connected to an AC electrical outlet by a power cord.
- CAT III : Primary electrical circuits of the equipment connected directly to the distribution panel, and feeders from the distribution panel to outlets.

Designed to meet CAT III 600V when the cap and protective cover is attached to the test lead and to meet CAT II 600V when the cap and protective cover is not attached to the test lead.

2. Features

This instrument is a pen-type digital multimeter and can measure: AC/DC voltage, resistance, capacitance and frequency/duty ratio. It also provides continuity check and diode check functions.


- Designed to meet the following safety standards. IEC61010-1 measurement category (CAT) III 600V IEC61010-031 (for hand-held Probe assemblies)
- Double molded main body and Function switch provide comfortable single handed grip.
- Penlight illuminates brightly the point to be measured.
- Backlight LCD is highly visible, even in darkness.
- REL function to check the difference (DCV/CAP).
- Auto-power-off function to save battery.
- Data hold function
- All ranges including Ohm range are protected against overload voltage of 600V.
- Test lead is wrapped in its rear side compartment without difficulty.
- Test pin can be covered by a unique cover mechanism for safety.

6-1 AC voltage(ACV), Frequency and DUTY ratio measurement

- Set the Function switch to \sqrt{V} position.
- Connect the Test pin and test lead to AC circuit as shown in the figure below to measure AC voltage (ACV).



- Press the SELECT key and select the Frequency range to measure a frequency. In this case, the unit "Hz" is displayed on the LCD.




- Press the SELECT key and select the DUTY ratio range to measure a DUTY ratio (Pulse width/ Pulse cycle). In this case, the unit "%" is displayed on the LCD.




Note
At ACV function, a few dgts may remain displayed on the LCD after removing the input.
Connect the test lead (minus terminal) to the earth side of the circuit under test. When the circuit under test does not have the earth, any connection is allowed.
At Frequency and DUTY ratio measurement, the measurable min. input is approx. 1.5Vrms.

6-2 DC voltage(DCV) measurement

- Set the Function switch to \sqrt{V} position.
- Connect the Test pin to the positive (+) side of the equipment under test and the test lead to the negative (-) side as shown in the figure below. When test lead is connected to the positive (+) side, the "±" mark is displayed on the LCD.



- Press the SELECT key to display a REL value (relative value). Press this key and store the initial measured value. After that, the difference between the stored value and the measured value is displayed on the LCD. Auto-ranging function doesn't activate when this function is enabled. The first selected range will be held. The relative measurement is allowed in the following range.
* Measuring range = Full scale value at a range - initial value
Press this key again or switch the measurement function to others to release the REL function.

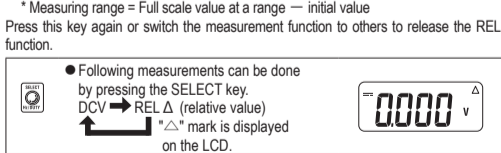

6-3 Resistance (Ω) measurement, Diode/ Continuity check

- Set the Function switch to Ω position.
- Connect the Test pin and test lead to the equipment under test as shown in the figure below.



3. Specification

Function	Range	Accuracy	Max. input voltage
ACV Auto-ranging(*2)	4V	±1.3%rdg ± 5dgt (50/60Hz)	DC 600V AC 600Vrms(sin)
	40V	±1.7%rdg ± 5dgt (~400Hz)	
	400V	±1.6%rdg ± 5dgt (50/60Hz)	
	600V	±2.0%rdg ± 5dgt (~400Hz)	
DCV Auto-ranging(*2)	400mV	±0.8%rdg ± 5dgt	
	4V		
	40V		
	400V		
Ω Auto-ranging	400 Ω	±1.0%rdg ± 5dgt	
	4k Ω		
	40k Ω		
	400k Ω		
Diode check/ Continuity Check	40M Ω	±2.5%rdg ± 5dgt	
	Diode check	Test voltage approx. 0.3V ~ 1.5V	
	Continuity Check	Buzzer sounds when resistance is 120 Ω or less.	
	Check	±3.5%rdg ± 10dgt	
Capacitance Auto-ranging	50nF	±3.5%rdg ± 5dgt	
	500nF		
	5 μ F		
	50 μ F		
Frequency Auto-ranging	100 μ F	±4.5%rdg ± 5dgt	
	5Hz	±0.1%rdg ± 5dgt Measurable input: 1.5Vrms or more	
	50Hz		
	500Hz		
5kHz			
DUTY(pulsewidth/ pulse cycle)	200kHz	±2.5%rdg ± 5dgt(Accuracy is guaranteed up to 10kHz.)	
	0.1 ~ 99.9%		

Note:
Following abbreviations are used in above table.
● **rdg** is an abbreviation of "reading", and it means the indicated value at a measurement.
● **dgt** is an abbreviation of "digit", and it means the figure to be displayed at the rightmost digit.
● (*) Except for 40M Ω range at Ohm function.
● (*2): At Voltage function, the Auto-ranging function is released by pressing the SELECT key. To measure a voltage again, turn the Function switch to the "OFF" position once. Then set it to the Voltage function again.

3-2 General specification

- Method of operation : Δ Σ method
- Display : Liquid crystal display (max. 3999 counts)/Units/ Marks
- Over-range indication : "OL" displayed when exceeding the measuring range. (Except for AC/DC 600V range)
- Range switching : Fully-automatic range (Single range is available at Continuity, Diode check and DUTY range.)
Range shifts to upper range:4000 counts or more.
Range shifts to lower range:less than 360 counts.
- Sample rate : twice per second
- Functional construction : OFF/ACV/DCV/ Ω /Capacitance
- Key : HOLD/Hz/DUTY/H/REL Δ (only at DCV and Capacitance ranges)
Button type battery LR44(SR44)1.5V x 2
"BATT" mark is displayed at 2.4V±0.2V or less.
- Power source : 190(L x 39(W) x 31(D)mm)
Approx. 100g (including batteries)
- Low battery warning : Altitude up to 2000m. in-door use
- Dimension : 0~40°C, relative humidity 85% or less (no condensation)
- Weight : -20~60°C, relative humidity 85% or less (no condensation)
- Location for use : Carrying case M-9130 x 1
Button type battery LR44(1.5V) x 2
Instruction manual x 1
- Operating temperature & humidity range : IEC/EN 61010-1, IEC/EN 61010-2-033
Measurement category (CAT) III 600V
Pollution degree 2
IEC/EN 61010-031
EN61326 (EMC)
- Storage temperature & humidity range : EU RoHS directive compliant
- Accessories : 3-3 Electrical characteristics


- Standards (Safety)
- Environmental standards : EU RoHS directive compliant
- 3-3 Electrical characteristics
- Temperature & humidity range : 23°C±5°C, relative humidity 85% or less (no condensation)
- Supply voltage range (guaranteed accuracy) : 3.4V till the "BATT" mark is displayed.
- Insulation resistance : 10M Ω or more/ DC1000V (between electrical circuit and case enclosure)
- Withstand voltage : AC150Vrms, sine wave (50/60Hz for 5 sec.) (between electrical circuit and case enclosure)
- Overload protection (Over-voltage protection) : 720V (AC/DC) for 10 sec. at voltage function
600V (AC/DC) for 10 sec. at all functions other than voltage function
- Rated supply voltage : DC3.0V
- Rated power : Approx. 4mVA (when battery voltage is 3.0V)
- Max. rated power : Approx. 30mVA (when lights are on)
- Continuous operating time : Approx. 80 hours (DCV measurement)
Approx. 15 hours (A operation; turning the light on for 10 sec. and off for 20 sec., is repeated.)

- Standards (Safety)
- Environmental standards : EU RoHS directive compliant
- 3-3 Electrical characteristics
- Temperature & humidity range : 23°C±5°C, relative humidity 85% or less (no condensation)
- Supply voltage range (guaranteed accuracy) : 3.4V till the "BATT" mark is displayed.
- Insulation resistance : 10M Ω or more/ DC1000V (between electrical circuit and case enclosure)
- Withstand voltage : AC150Vrms, sine wave (50/60Hz for 5 sec.) (between electrical circuit and case enclosure)
- Overload protection (Over-voltage protection) : 720V (AC/DC) for 10 sec. at voltage function
600V (AC/DC) for 10 sec. at all functions other than voltage function
- Rated supply voltage : DC3.0V
- Rated power : Approx. 4mVA (when battery voltage is 3.0V)
- Max. rated power : Approx. 30mVA (when lights are on)
- Continuous operating time : Approx. 80 hours (DCV measurement)
Approx. 15 hours (A operation; turning the light on for 10 sec. and off for 20 sec., is repeated.)


- Standards (Safety)
- Environmental standards : EU RoHS directive compliant
- 3-3 Electrical characteristics
- Temperature & humidity range : 23°C±5°C, relative humidity 85% or less (no condensation)
- Supply voltage range (guaranteed accuracy) : 3.4V till the "BATT" mark is displayed.
- Insulation resistance : 10M Ω or more/ DC1000V (between electrical circuit and case enclosure)
- Withstand voltage : AC150Vrms, sine wave (50/60Hz for 5 sec.) (between electrical circuit and case enclosure)
- Overload protection (Over-voltage protection) : 720V (AC/DC) for 10 sec. at voltage function
600V (AC/DC) for 10 sec. at all functions other than voltage function
- Rated supply voltage : DC3.0V
- Rated power : Approx. 4mVA (when battery voltage is 3.0V)
- Max. rated power : Approx. 30mVA (when lights are on)
- Continuous operating time : Approx. 80 hours (DCV measurement)
Approx. 15 hours (A operation; turning the light on for 10 sec. and off for 20 sec., is repeated.)

3. Press the SELECT key to conduct the Diode check.

Connect the Test pin and the test lead to the equipment under test. When following indication is confirmed, the diode is good.



- Forward direction
- Backward direction



Note
When the forward voltage of diode is out of the range of 0.3V~1.5V, measurement may not be done. (Zener diode, LED and etc.)

4. Press the SELECT key to conduct the Continuity check.

Connect the Test pin and the test lead to the equipment under test. Buzzer sounds when continuity is ok. (120 Ω or less) Resistance value of 400 Ω or less is displayed on the LCD.




Note
Indicated value may not be "0" after shorting the tip of the test lead. However, this is because of the resistance of the test lead and not a failure.

6-4 Capacitance measurement (nF, μ F)

- Set the Function switch to \sqrt{F} position.



- Press the SELECT key to make the indicated value to "0" before connecting the test lead to the equipment under test.



- Connect the Test pin and the test lead to the equipment under test as shown in the figure below.




Note
Measuring time varies depending on the capacitance to be measured.

Capacitance to be measured	< 4 μ F	< 40 μ F	< 100 μ F
Measuring time	2 sec.	7 sec.	15 sec.


4. Instrument layout

4-1 Instrument layout

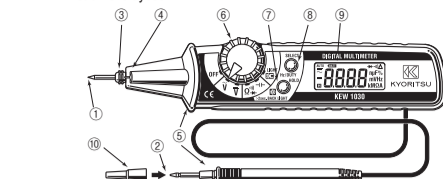

- Test pin (input terminal (+): red)
- Test lead (input terminal (-): black)
- Connected to the negative (-) side or the earth of the circuit.
- Protective cover
- Covering the Test pin for safety purpose.
- Penlight
- Protective fingerguard : It is a part providing protection against electrical shock and ensuring the minimum required air and creepage distances.
- Function switch

- OFF : Power off (Battery will not be wasted)
- V AC voltage (ACV) \rightarrow Frequency (Hz) \rightarrow DUTY(%)
Switches by pressing the "SELECT" key.
- V DC voltage (DCV) \rightarrow REL Δ (relative value display)
Switches by pressing the "SELECT" key.
- Ω Resistance \rightarrow Diode check \rightarrow Continuity check
Switches by pressing the "SELECT" key.
- \sqrt{F} Capacitance \rightarrow REL Δ (relative value)
Switches by pressing the "SELECT" key.
- LIGHT : Turning on the Penlight. Set the Function switch to this position first, and then turn it to any desirable function position. Then the Penlight turned on and illuminates the test point. (Measurement cannot be performed in this switch position.)
- HOLD key : Freezing the indicated value.
Turning on the LCD backlight. (Press this key at least 2 sec.)
- SELECT key : Switching the measurement modes. (V / Hz/ DUTY and Ω / \sqrt{F})
Enable/Disable the REL Δ function. (Only at DCV/ Capacitance)
- LCD indication

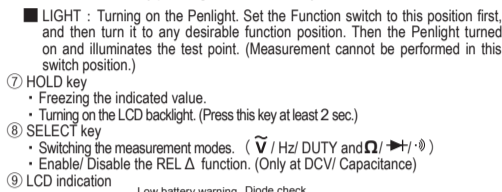

- Cap : Test leads can be used under the CAT II and CAT III environments by attaching a protective cap as illustrated below. Use of our protective cap offers different lengths suitable for the test environments. When the instrument and the test lead are combined and used together, whichever lower category either of them belongs to will be applied.


4-2 Protective cover

CAUTION

- Do not apply excessive force to the Test pin and the Protective cover.
- Be careful not get hurt by the tip of the Test pin when setting or releasing the Protective cover.
- Designed to meet CAT III 600V when the cap is attached to the test lead and to meet CAT II 600V when the cap is not attached to the test lead.

Use the Protective cover to cover the Test pin when carrying or storing the instrument.

1. Method of setting the Protective cover
Pinch the tip of the Protective cover, and pull it towards the tip direction. Then turn it 90 degrees as shown in the figure below to match the marks on the cover and on the instrument body.



2. Method of releasing the Protective cover
Pinch the tip of the Protective cover, and pull it towards the tip direction. Then turn it 90 degrees as shown in the above figure. Then the cover is stored automatically and the Test pin (positive terminal) appears.

7. Battery replacement

WARNING

- To avoid getting electrical shock, be sure to remove the measuring terminals from the equipment under test; set the Function switch to OFF position before replacing batteries.


DANGER

- Do not mix new and old batteries. Never mix the different kinds of batteries.
- Make sure to install batteries in correct polarity as marked inside.
- Be sure to fasten the Battery case-fixing screws after the battery replacement.

CAUTION

- Dispose the used batteries according to the rules, which are defined by each community.

- Set the Function switch to OFF position.
- Loosen one Battery cover-fixing screw, and remove the Battery cover.
- Replace the batteries with new ones. Make sure to install batteries in correct polarity as marked inside. Always replace all two batteries with new ones at the same time.
- Put the Battery case at the original position, and fasten the screws.

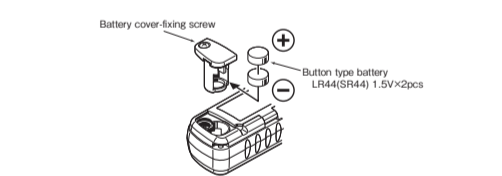

8. Maintenance

- Cleaning**
Use a cloth dipped in water or neutral detergent for cleaning the instrument. Do not use abrasives or solvents. Otherwise, instrument get damaged, deformed or discolored.

DISTRIBUTOR

Kyoritsu reserves the rights to change specifications or designs described in this manual without notice and without obligations.

KYORITSU ELECTRICAL INSTRUMENTS WORKS, LTD.
2-5-20, Nakane, Meguro-ku, Tokyo, 152-0031 Japan
Phone: +81-3-3723-0131
Fax: +81-3-3723-0152
Factory: Ehime, Japan
www.kew-ltd.co.jp